


# MASS SPECTROMETRY REPORT

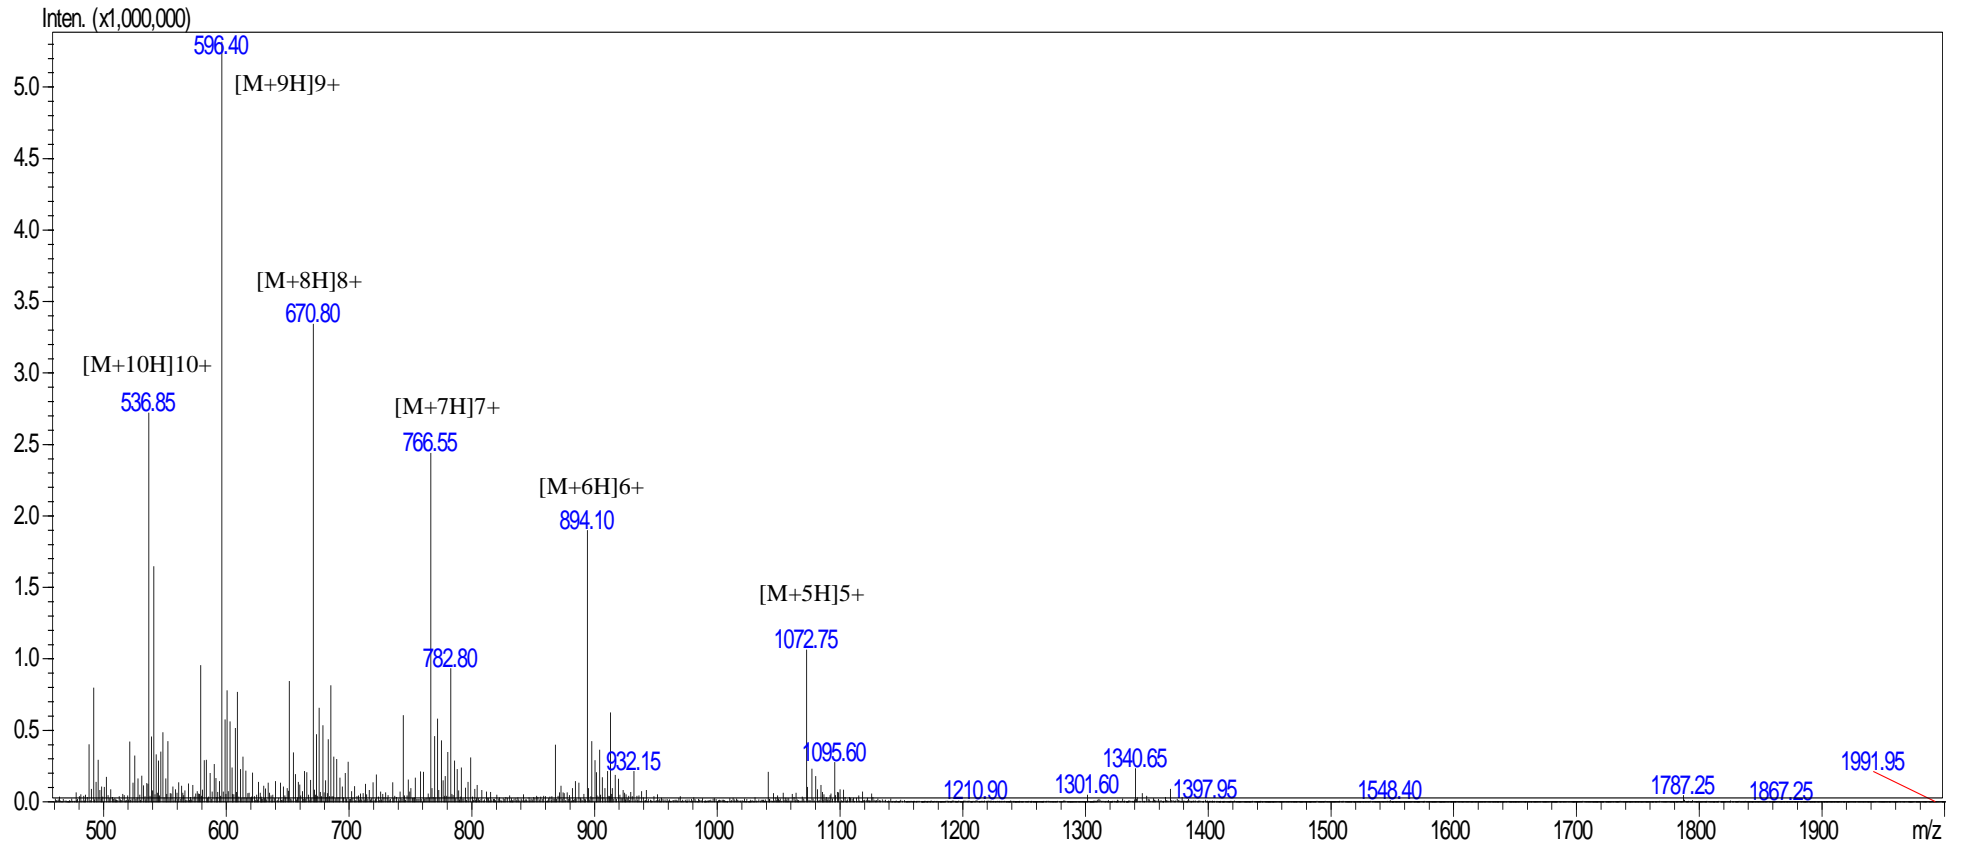

## Sample Description

Analyzed date: 2017/12/7

Analyst: Shen

Sample: LG-46

M.W.: 5358.05

Lot. No.: NJP20501-171106

## Instrument

Probe:

Nebulizer Gas Flow:

CDL:

CDL Temp.:

Block Temp.:

SHIMADZU LCMS-2020

ESI

1.5L/min

-20.0v

250 °C

400 °C

Probe Bias:

Detector:

T. Flow:

B. Conc.:

+4.5kv

1.2kv

0.2ml/min

50% H<sub>2</sub>O/50% ACN